


Marker Bands

Merit Medical's technology impregnates polyurethane marker bands with Tungsten, Platinum or other precious metal powder to create a tough and flexible marker band that is visible under fluoroscopy.

CUSTOM
BUILT TO ORDER

- Catheter shaft OD range of 0.022" to 0.270"
- Wall thickness down to 0.006"
- Ideal for polyurethane catheters

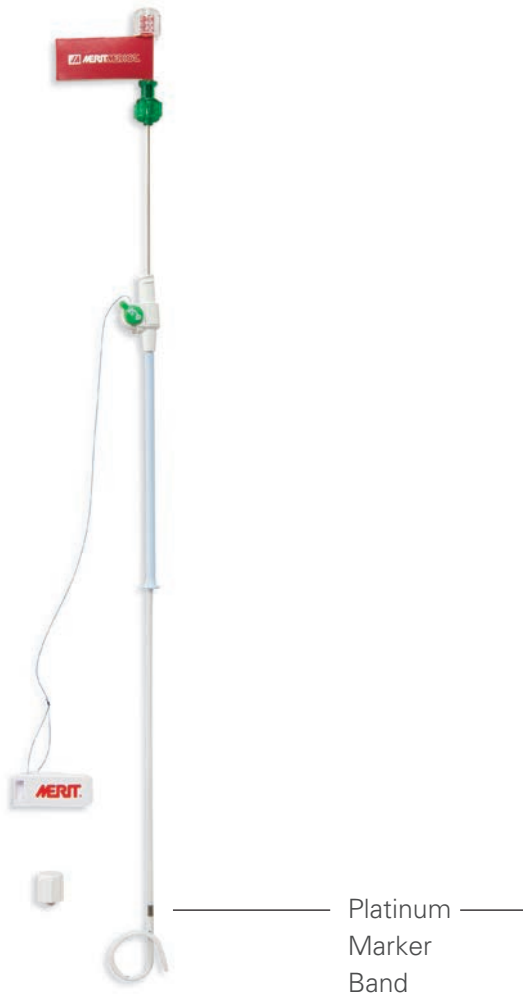

Used in Merit's own
Drainage Catheter Line

CATHETERS
& EXTRUSIONS